MIDMARK®

Installation Instructions

9A97002 Foot Control

and 9A98002 Foot Control

(1) Unpack the foot control and inspect it for shipping damage. If you detect damage, contact the shipping carrier and Midmark immediately.

(2) Before installing the foot control, review the operating procedures outlined in the table's installation & operation manual: 9A97002 - Model #417; 9A98002 - Model #414.

(3) Insert the coil cord into both the foot control and the control port at the base of the table.

(4) Test the foot control before putting the table back into service.

Clean the foot control periodically with a damp cloth and a mild soap solution. Always unplug the foot control coil cord from the table prior to cleaning and never immerse in water or other fluids.

If you have questions concerning the operation of your table or in the event of equipment failure, please contact your dealer. If you can't resolve your problem through your dealer, call Midmark at 1-800-MIDMARK.

9A98002 FOOT CONTROL - MODEL #414

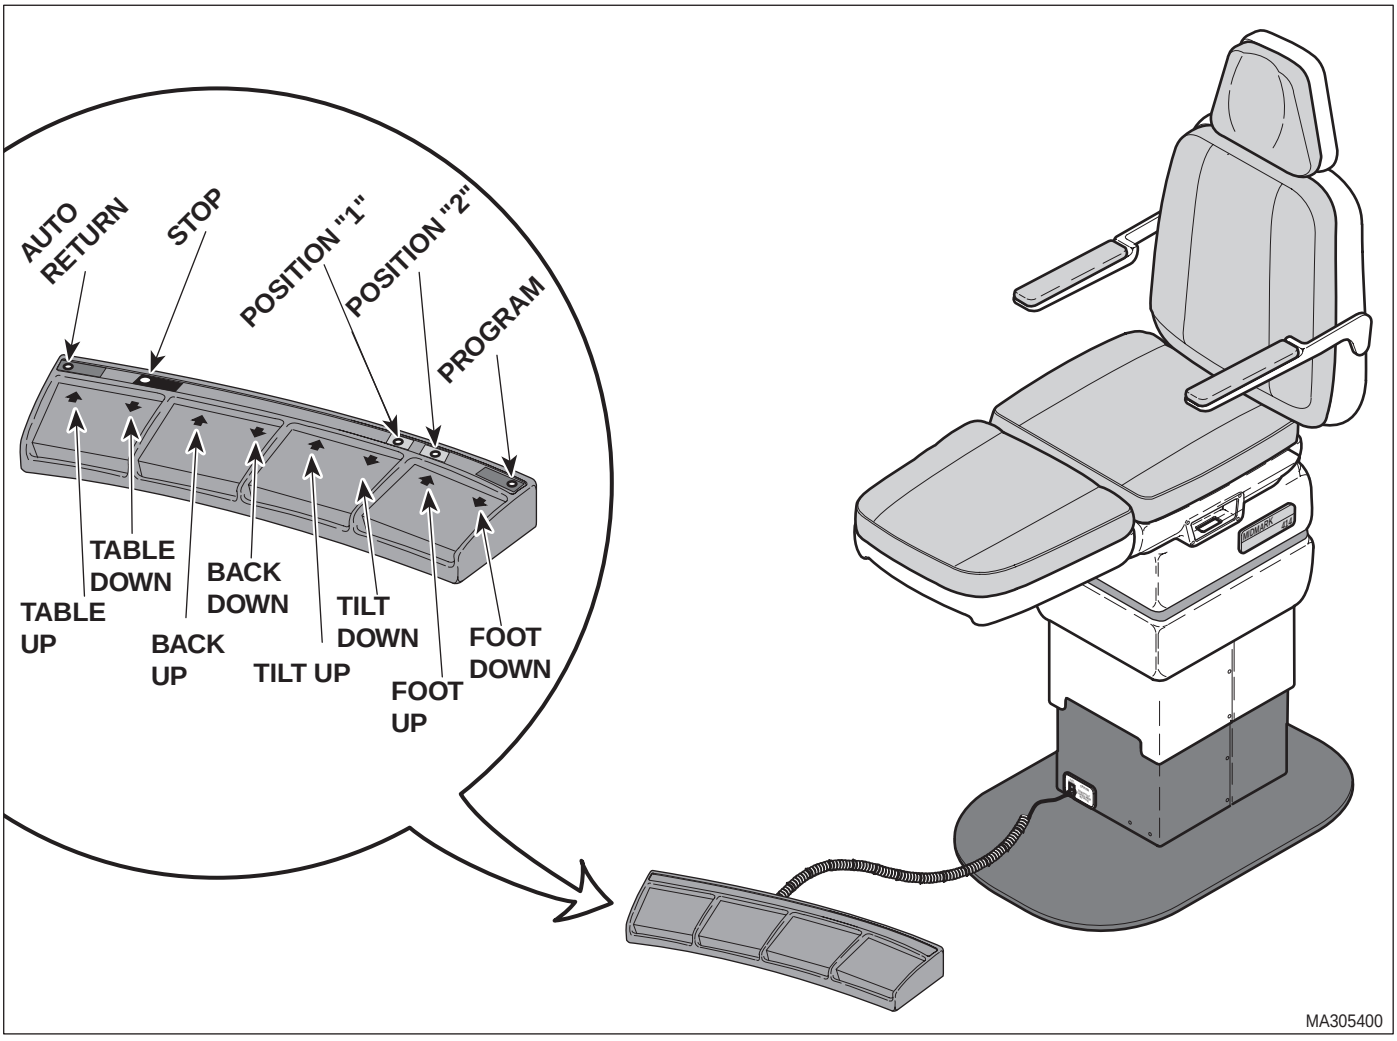

9A97002 FOOT CONTROL - MODEL #417

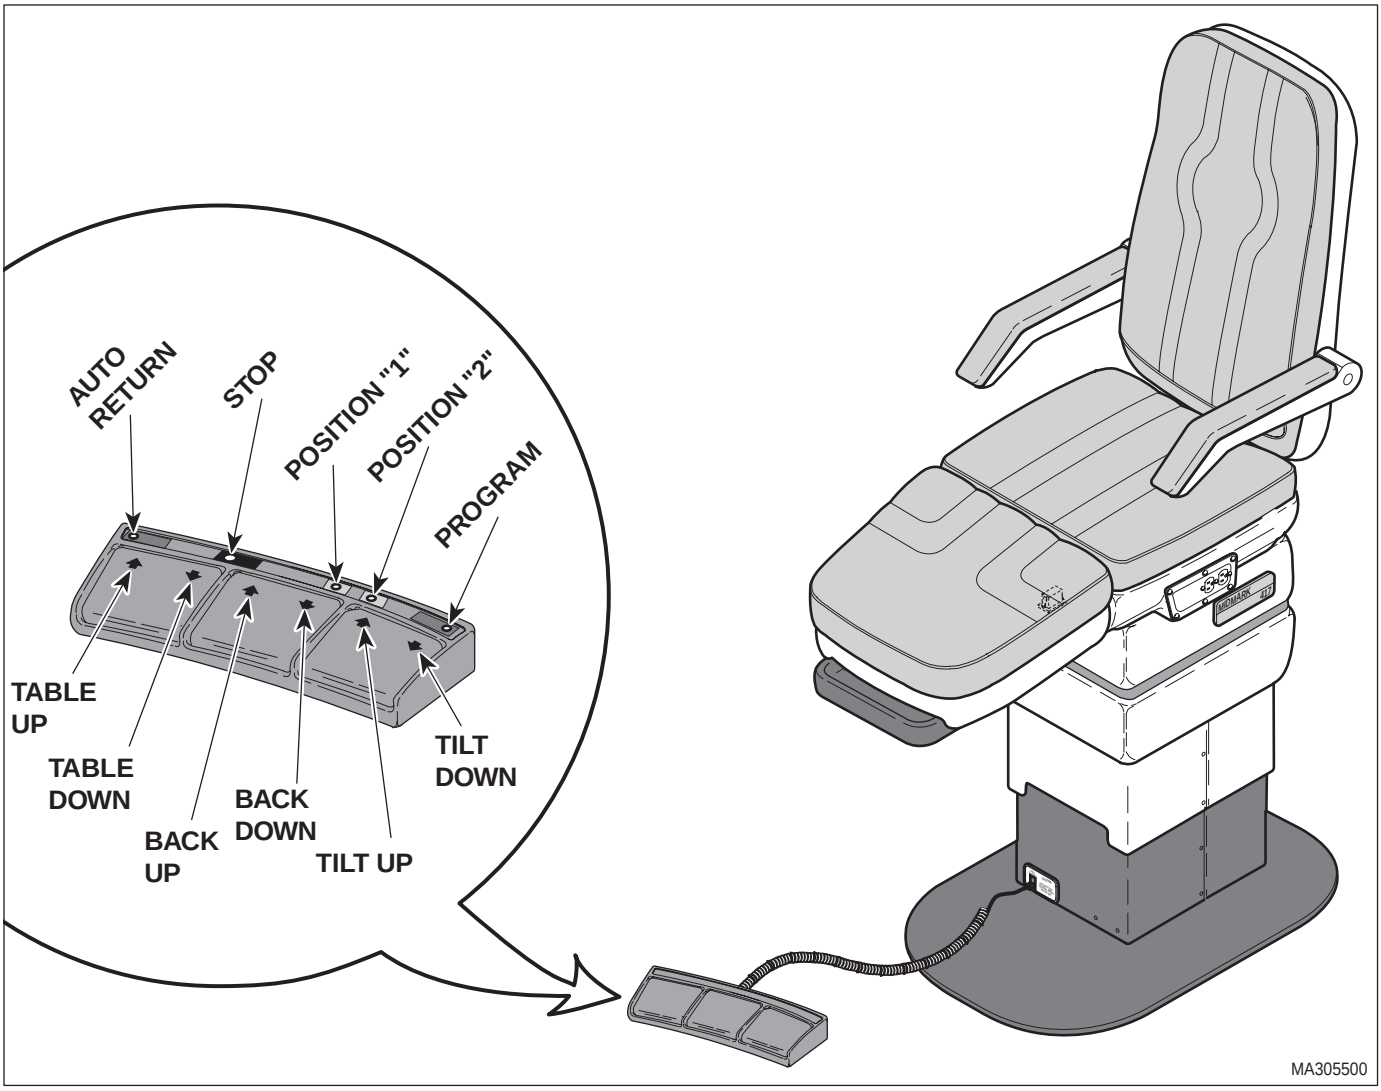

© Midmark Corporation - 1996

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
937-526-3662 TELEX 288007 FAX 937-526-5542